


Operating Manual

Probe Ultrasonicator

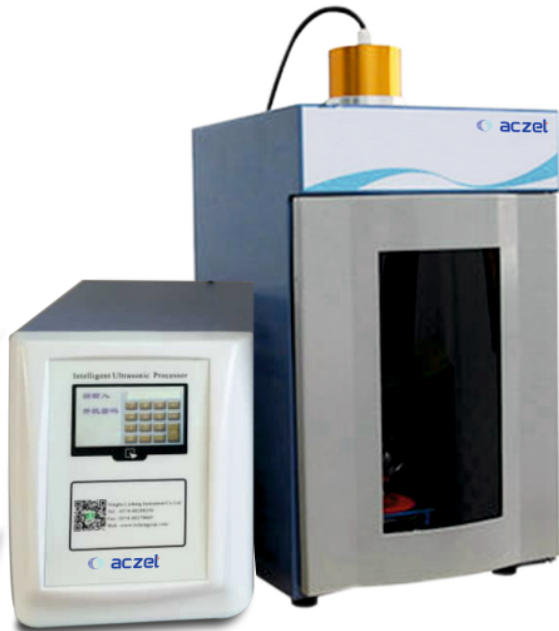

APU series

I. General Description

4.3 inch TFT touch screen series ultrasonic homogenizer sonicator is our company's new developed product. With full functions, beautiful appearance, reliable performance. Instrument using large LCD display screen, using the central computer centralized control system, ultrasonic output, gap time, ultrasonic power, duty cycle, temperature can be arbitrarily set, sample detection temperature display, frequency automatic tracking, automatic fault alarm.

II. Functions and composition

2.1 Our ultrasonic homogenizer sonicator is a multi-function and multi-purpose instrument that utilizes ultrasonic cavitation in liquid. It can be used for breaking many kinds of cells, bacteria, viruses, animal and plant tissues, also for emulsification and separation, homogenization, extraction, defoaming, cleaning, preparation of nanomaterials, dispersion and accelerated chemical reactions. Widely used in biology, medicine, agriculture, chemistry, materials science, pharmaceutical and other fields of teaching, research, production.

2.2 This machine consists of ultrasonic generator (power), transducer components and sound proof box, middle part connected by the cable

III. Precautions before use

3.1. Check power supply: This machine is powered by $220V \pm 5\%$ AC voltage (frequency 50Hz), the power socket is located in the lower left of the instrument rear panel. Please pay attention to the color of the power supply are fitted at the left lower sections of the backboard.

Warning: Please kindly use grounded AC power supply to avoid lightning and for safe using, and remove the plug when replacing the fuse

3.2 Working environment

The instrument should be placed in a well ventilated place to work, the normal working room temperature range is 0 °C to 40 °C.

**In order to ensure that the instrument can work normally, please kindly note:
Anti-corrosion, moisture-proof, sun protection, dust prevention**

3.3 Installation

- Connect the power cord, transducer and temperature probe according to each socket

- Insert the transducer into the soundproof box and select suitable container according to the sample size, pour the sample and put it on the lifting platform of the sound proof box. adjust the lift height, the end of the horn inserted into the sample surface is generally 10-20mm and make it in the center of the container.

The horn can not touch the wall of the container, the end part of horn and the bottom of the container should be more than 4cm(or will case no load when with bigger power), to ensure the good break effect

Recommended for use elongated containers.when process small capacity samples, using small ultrasonic power, the horn never can contact with the bottom of the container.


IV. Scope of application for various specifications of horns and the best power ratio for new instrument as follows:

Horns (mm)	Φ2	Φ3	? Φ6	Φ8	Φ10	Φ12
Process capacity (ml)	0.2-5	3-10	10-100	20-200	30-300	50-500
Power ratio (1-99%)	1-35%	1-45%	1-60%	1-70%	10-90%	20-95%

V. Function and main parameters


1. For the first time use, add water in a 50ml beaker, then put it on the lifting table of the sound proof box, place the transducer on the top hole of the sound proof box, adjust the lift to make the liquid surface immersion horn end face 1-2cm
2. Connect the power supply, temperature, transducer interface of the ultrasonic generator, turn on the power switch on the back of the instrument.
3. Click the password box after turn on the machine, then type "123456" to enter the factory standby state (usually remove the password before leaving the factory),

Please see below diagram "standby interface A"

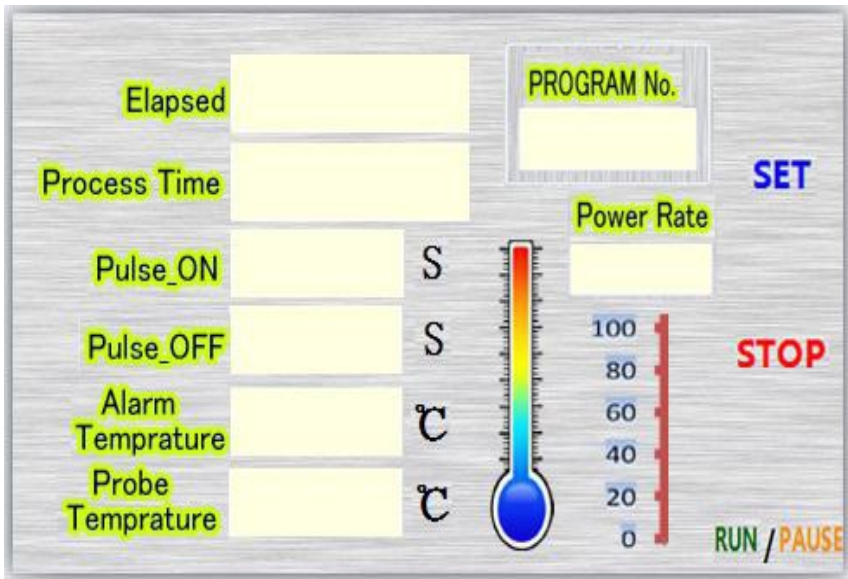

"Standby interface A"

4. Check if the the horn size on the screen consistent with the actual one, if need to reset, please click "SET" button, enter the setting state, as shown in the following figure "Setting interface B", at this time can modify the parameters according to your requirement, click on the box to set your needed parameters, modify it when the numeric keypad jump out, usually can not set "0"

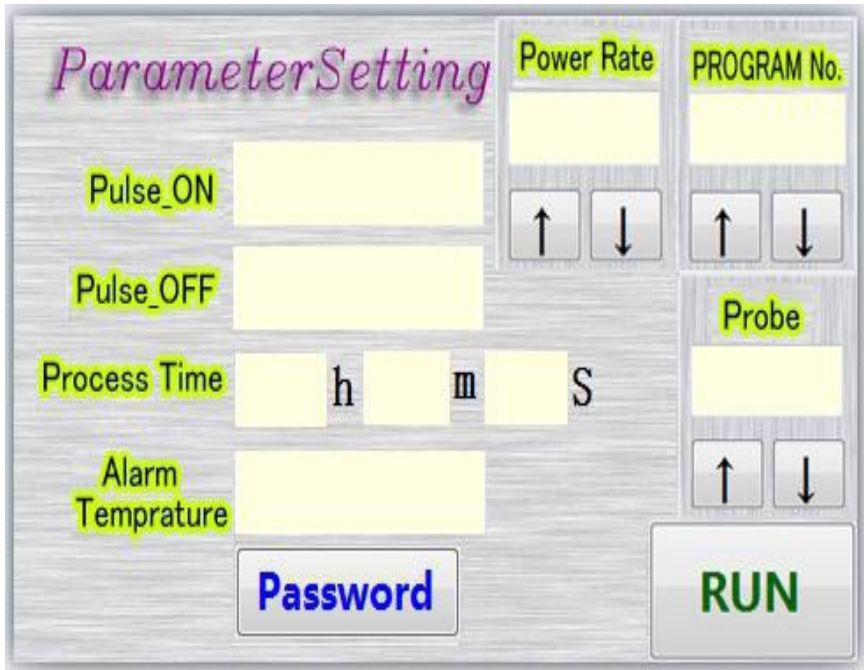

"Setting interface B"? The choice of horn should consistent with the actual installation horn's size?


5. After setting the parameters and click the "RUN" button, the interface into standby state, then click the "RUN" button again, the instrument begin to work, if need to stop the ultrasound can click the "PAUSE" button, If one cycle of work finished, you need to continue to work, please click "STOP" button, then click "RUN" button, in order to ensure user's experimental data preservation, this instrument has 20 sets of parameters stored (0-19) and call function, adjust above "settings interface B " PROGRAM No." is ok

6. If the "RESET" key box becomes yellow when the instrument on the working process, it's for over-temperature alarm, please check whether the set temperature is too low, It's for overload or fault alarm if turn into red color, then click the "reset" key box cancel the alarm

7. Main technical parameters of the instrument

Output power	10-650W (adjustable)
Working frequency	20-25KHz frequency automatic tracking
Process capacity	0.2-500ml (need to match corresponding probe)
Timing	0-99H59M59S (can be set)
Working mode	Pulsed
Pulse	0.1-99.9s adjustable? interval/working?
Temperature control	Control samples' temperature? 0°C-100°C)
Alarm	Fault, temperature, time
Input method	touch screen control,
Display method	touch screen control, 4.3 inch TFT
Display content	Temperature, power, time, etc.
Protective device	Program automatic error correction, overload, over temperature protection display
Storing data	20 groups
password	Have user password protection
Standard configuration	Ultrasonic generator (host) one set Sealed transducers + 6MM horn one set Φ6mm? process capacity 10ml-100ml?
Optional horn	Φ2, Φ3, Φ8, Φ10, Φ12
Power supply (AC)	220V±5% /50Hz(can customize 110V)

Instrument interface description(Rear panel)

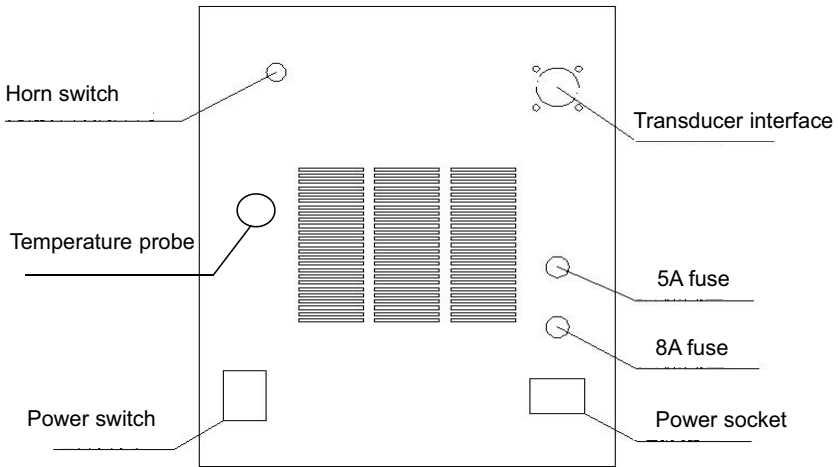

VI. Instructions

5.1 Cautions

1. Temperature protection set point should be **1-3°C higher** than the room temperature or the sample temperature. machine will stop in case of over-temperature.

2. **Don't start the machine when the horn is not inserted into the liquid (no load)**, otherwise it will damage the instrument

3. Process capacity, ultrasonic time&power, waiting for user explore according to a variety of different cells and select the best value

4. After using a long time, the end of the horn will be cavitation corrosion and hairy, can use oil stone or file make it flat, otherwise will affect the work effect

5. In the working process, due to ultrasonic cavitation in the liquid effect, the liquid

temperature will rise rapidly, the user should pay more attention to the temperature of various cells, recommended to use short ultrasonic time (less than 5 seconds each time) while also can connect cooling bath for cooling (**ultrasonic time 1-4 seconds and gap time 2-8 seconds**)

Warning: Turn off the power supply when you change the horn. Please re-select correct horn specification on the interface after restart; otherwise it may cause horn to be damaged

KIND REMIND:

★ Practices prove that instrument will have a better performance at working 1~3 seconds and interval 2~6 seconds. you may set a longer gap time to avoid liquid temperature increase. In addition, continuous working may cause empty load, will shorten the life of the instrument
Φ6mm horn's maximum output power should not exceed 80% for new instrument

? Horn selection switch at the back of the machine(must be same as the actual installation of horn for new machine) ?

? NOTE: Please select correct horn (size), for example interface displays φ6, then you must select φ6 horn. And the switch at the back panel for horn shall be also φ6.

★After the horn is used for a long time, when appear honeycomb, make it flat with file. if the ultrasonic wave can not be generated normally, you can change the horn switch on the back board until the ultrasonic wave is normal.
if the ultrasonic wave can not be generated normally when open the machine (voltage instability or external interference, can change the horn switch on the back board until the ultrasonic wave is normal

VII. Removal and installation horn Diagram 3

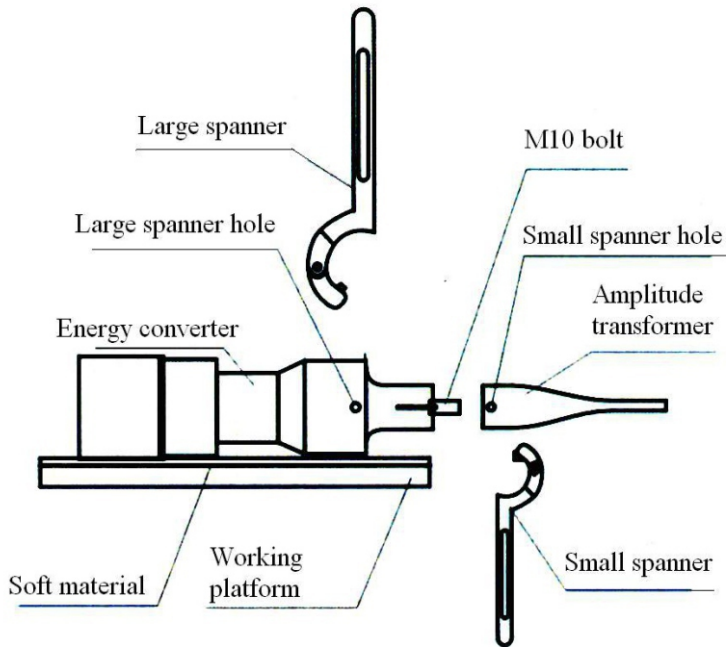


Diagram 3 Removal and installation horn

- Push the energy converter on the chair with soft materials (such as towel). Put the small spanner into the horn spanner hole and the large spanner into the transducer spanner hole. the large and small spanners shall be oriented to the left and right.
- You stand facing the horn, and hold the large spanner with left hand and small spanner with right hand. Tighten downward with both hands(**must be tightened**)
- When changing the horn, such as the M10 screw on the horn, remove the bolt out by hand, and then fasten the bolts on the transducer, and **must be tightened**. If the bolts on the horn, Hex wrench can not be twisted, you can knock the bolts on the wood materials for a few times then can twist

VIII. Examples of experimental data for some samples

? please refer to Φ 6mm horn?

Experimental sample	Ultrasonic time (S)	interval time (S)	Total working time? Minute?	Power ? %?	container ? ml?	Broken rate ? %?
Treponema pallidum	1.5	2	10—20	30	20	Above 90
staphylococcus	1.5	2	10—25	30	20	Above 90
Mouse sciatic nerve	2	3	10—15	30	20	Above 92
Mouse liver	2	3	5—15	45	30	Above 95
Liver cell enzyme extraction	2	3	5—10	50	30	Above 95
Escherichia coli	2	3	10—15	50	50	Above 93
Pseudomonas aeruginosa	2	3	5—10	60	50	Above 92

VIII. Packing list

1. Ultrasonic generator 1 set
2. Sonic system (transducer components+ 6mm horn) 1set
3. Sound proof box (another package 1 pc
4. Lift table (inside of sound proof box) 1 pair
5. Power cable 1pc
6. Fuse (Inside the power cord bag) 2 pcs
7. User manual 1pc
8. Warranty card (include product certificate) 1 copy
9. Temperature probe 1pc

Qualified product after inspection, allowed for output.

Probe Ultrasonic

APU Series

Model	APU 250	APU 500
Frequency (Khz)	20-25KHz Automatic Tracking	
Power (W) adjustable	5-250W	10-500W
Probe (mm)	Ø 6	
Optional Probe (mm)	Ø2, Ø3, Ø8, Ø10	Ø2, Ø3, Ø8, Ø10, Ø12
Process Capacity (ml)	0.2-250	0.2-500
Store Data	50 sets	
Total Working Temperature	1-999 minutes	
Temp. Alarm Range	0-100°C	
Instrument Protection Function	Over-temp.	
Duty Ratio	0.1-99.9%	
Display	Touch Screen Display	
Power Requirements	230 Vac, ± 20%, 50-60Hz	
Dimension (LxWxH)	600 x 300 x 500mm	
Weight Approx.	30 kg	

LIMITED WARRANTY

ACZET products are warranted against defects in materials and workmanship from the date of delivery through the duration of the warranty period. During the warranty period Aczet will repair, or, at its option, replace any components(S) that proves to be defective at no charge, provided that the product is returned, freight prepaid, to ACZET.

This warranty does not apply if the product has been damaged by accident or misuse, exposed to radioactive or corrosive materials, has foreign material penetrating to the inside of the product, or as a result of service or modification by other than ACZET. In lieu of a properly returned warranty registration card, the warranty period shall begin on the date of shipment to the authorized dealer. No other express or implied warranty is given by Aczet Pvt. Ltd.

As warranty legislation differs from state to state and country to country, please contact aczet or your local ACZET dealer for further details.

ACZET service center will repair the product free of charge subject to terms & condition mentioned below.

TERMS & CONDITION

- 1.It covers only weighing balance purchased from authorized channel and does not covers accessories like Battery, Adaptor, RS232 cable, Pan, Pan support etc
- 2.It does not cover the product of which model and serial number has been altered, removed or defaced and / or is open by unauthorized person and found void sticker has been tampered.
- 3.This warranty is non-transferable and applicable only to first end user purchasing the product from authorized dealer.
- 4.For repair based on this warranty you need to hand over this product or send this product to address mentioned in warranty card in original packing, enclosing copy of this warranty card.
- 5.Aczet Pvt. Ltd. shall not be liable for any consequential damages.

WARRANTY REGISTRATION



ACZET PVT.LTD.
E2, Plot No. 15, WICEL Estate,
Opp. Seepz Gate No. 1,
Andheri (E), Mumbai 400 093
E-mail : service@aczet.com
web: www.aczet.com
Tel. No. : +91 22 4243 7700
Fax No. : +91 22 4243 7800

NAME :-

ADDRESS :-

TEL NO. :- MODEL NO. :-

SERIAL NO. :- PURCHASE DATE :-

BRANCH / DISTRIBUTOR / DEALER CONTACT DETAILS

WARRANTY PERIOD :-

STAMP / SIGN

Owners Signature / Date

SEND YOUR WARRANTY CARD DULY FILL TO ABOVE ADDRESS FOR REGISTRATION